


## Single-Patient Use Proper Cuff Placement Guide


### Step 1

Place the microphone into the microphone pad as shown. The adhesive surface will keep the microphone inside the microphone pad.

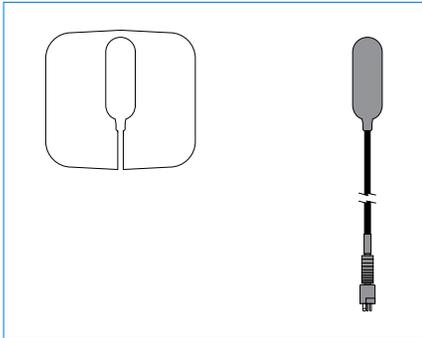


### Step 2

Peel off the protective covering on the microphone pad as shown below.

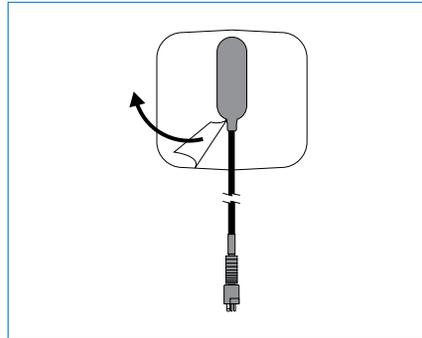


### Step 3

Microphone placement is essential to the performance of the *Tango+*. Place the microphone over the brachial artery, in between the bicep and tricep muscles (approximately the width of 2 fingers above the elbow crease).

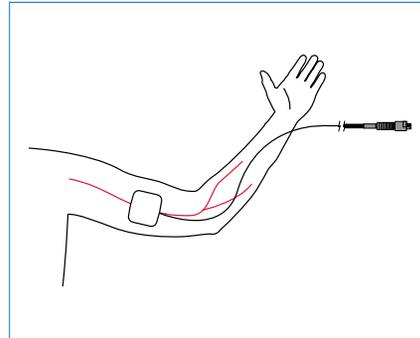


### Step 4

Choose the appropriately-sized *SunTech* disposable cuff. The cuff has range markers on both the inside and outside to ensure proper sizing.

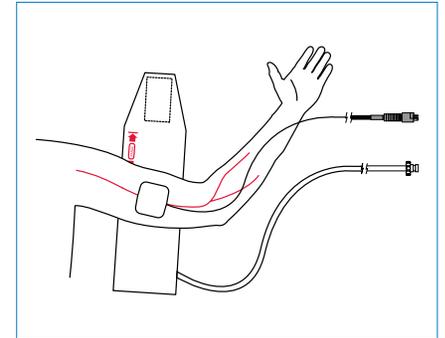


### Step 5

Wrap the cuff securely around the arm. The artery marker should be over the brachial artery as shown below.

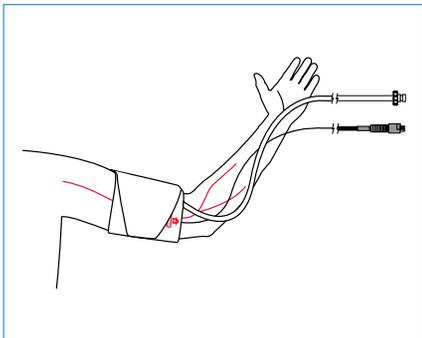


### Step 6

Insert the microphone cable into the connector as shown below. Note there is only ONE way to insert the microphone into the connector.

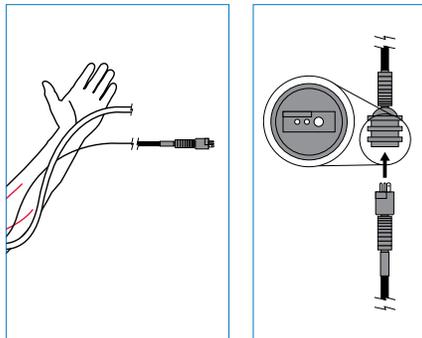


### Step 7

Connect the cuff hose to the patient cable connector of the *Tango+* patient cable as shown below.

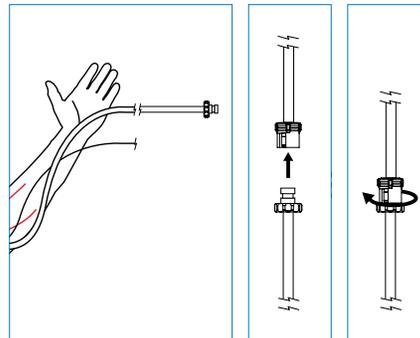

### Step 8


Use the wrist straps provided with the *Tango+* system to secure both the patient cable and the microphone cable to the patient's wrist as shown below.

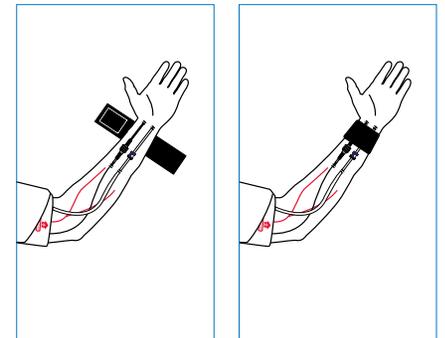

## Single-Patient Use Proper Cuff Placement Guide


### Step 1

Place the microphone into the microphone pad as shown. The adhesive surface will keep the microphone inside the microphone pad.

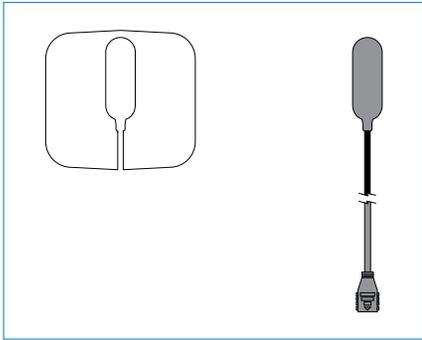


### Step 2

Peel off the protective covering on the microphone pad as shown below.

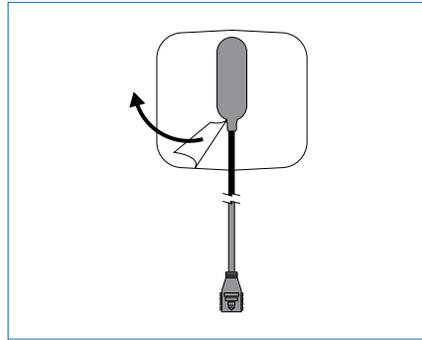


### Step 3

Microphone placement is essential to the performance of the *Tango M2*. Place the microphone over the brachial artery, in between the bicep and tricep muscles (approximately the width of 2 fingers above the elbow crease).

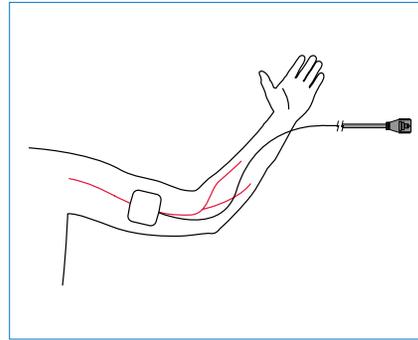


### Step 4

Choose the appropriately-sized *SunTech* disposable cuff. The cuff has range markers on both the inside and outside to ensure proper sizing.

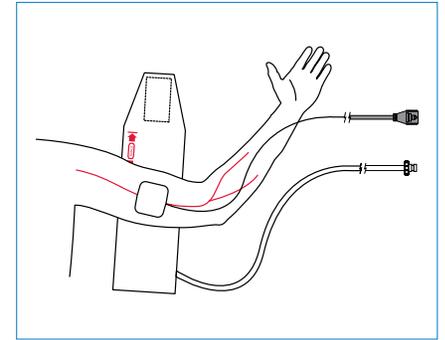


### Step 5

Wrap the cuff securely around the arm. The artery marker should be over the brachial artery as shown below.

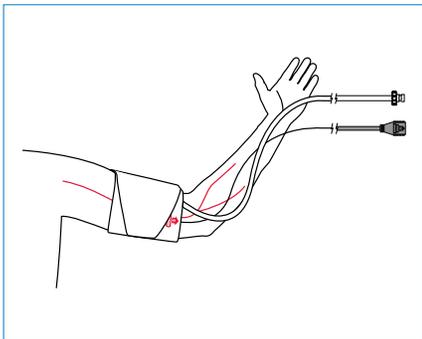


### Step 6

Insert the microphone cable into the connector as shown below. The connectors can be inserted in any orientation. An audible click will be heard when a secure connection is made.

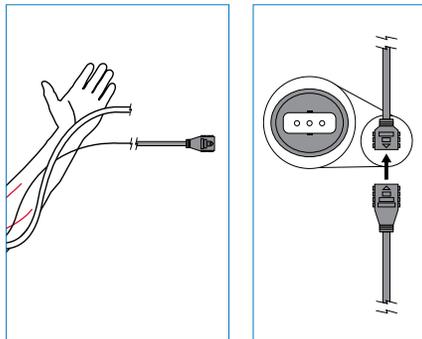

### Step 7

Connect the cuff hose to the patient cable connector of the *Tango M2* patient cable as shown below.

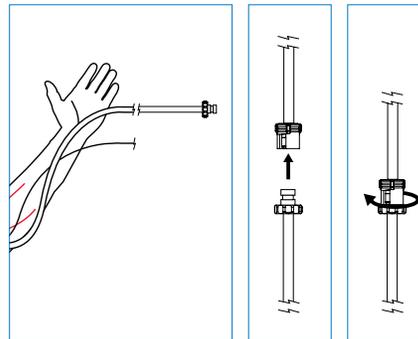

### Step 8

Use the wrist straps provided with the *Tango M2* system to secure both the patient cable and the microphone cable to the patient's wrist as shown below.

