


Orbit-K™ Proper Cuff Placement Guide


Step 1

Palpate the brachial artery between the tricep and bicep.

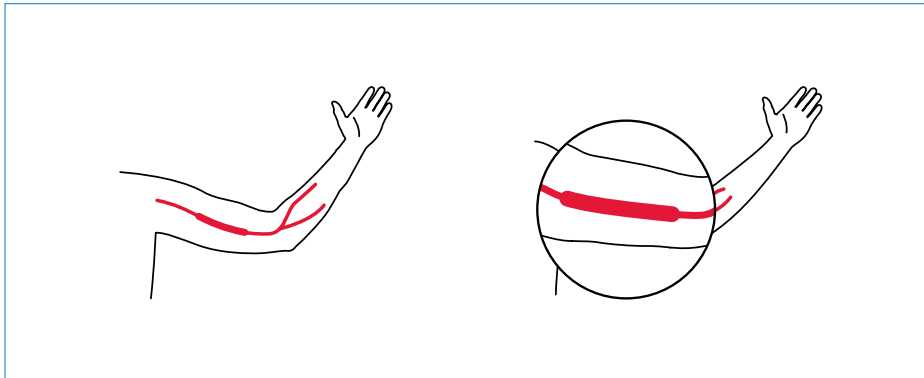


Step 2

Choose the appropriate size cuff. The cuff has range markers on both the inside and outside to ensure proper sizing.

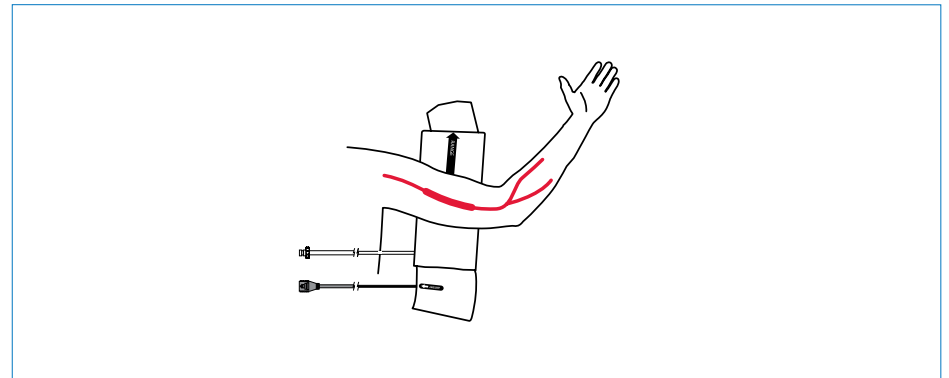


Step 3

Place the cuff on the arm. Ensure the artery marker points down the arm and the microphone is placed over the brachial artery, 3-5 cm from the elbow.

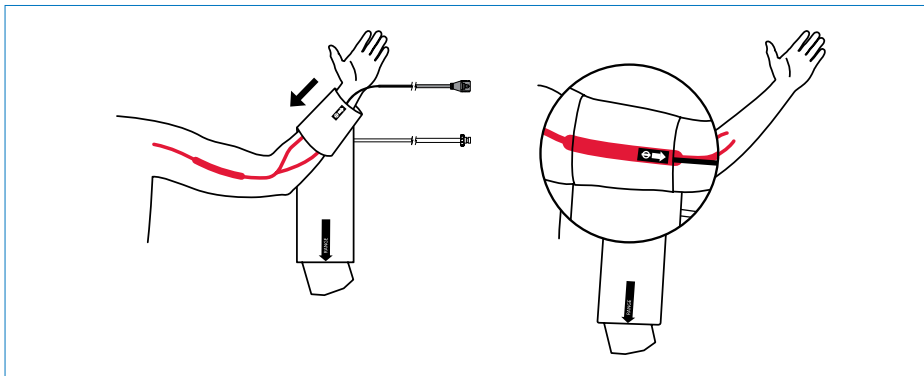

Step 4


Wrap the cuff securely around the arm. Use the wrist straps provided with the *Tango* M2 system to secure both the patient cable and the microphone cable to the patient's wrist as shown below.

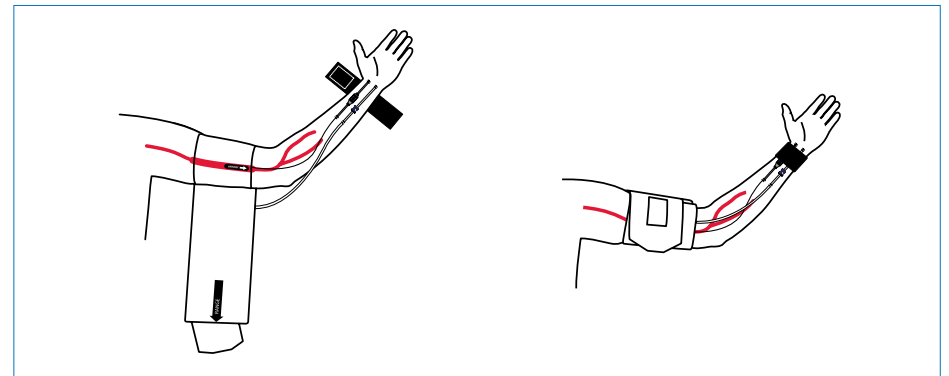

Single-Patient Use Proper Cuff Placement Guide


Step 1

Place the microphone into the microphone pad as shown. The adhesive surface will keep the microphone inside the microphone pad.

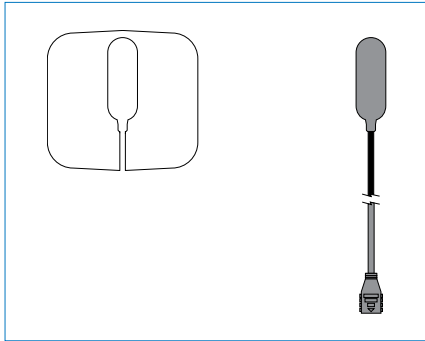


Step 2

Peel off the protective covering on the microphone pad as shown below.

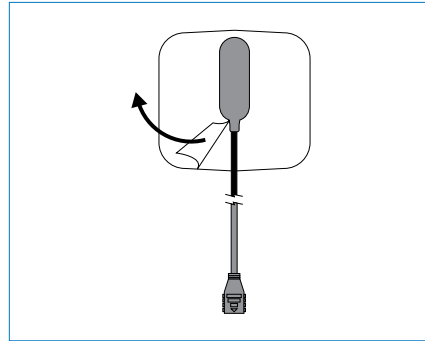


Step 3

Microphone placement is essential to the performance of the *Tango M2*. Place the microphone over the brachial artery, in between the bicep and tricep muscles (approximately the width of 2 fingers above the elbow crease).

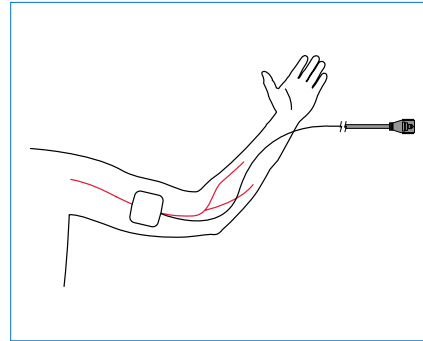


Step 4

Choose the appropriately-sized *SunTech* disposable cuff. The cuff has range markers on both the inside and outside to ensure proper sizing.

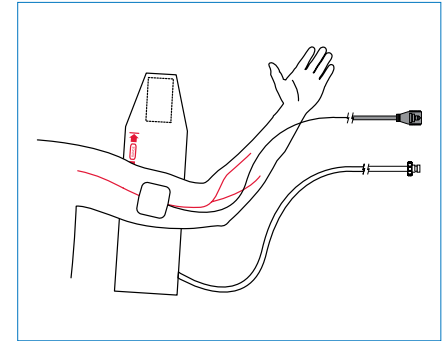


Step 5

Wrap the cuff securely around the arm. The artery marker should be over the brachial artery as shown below.

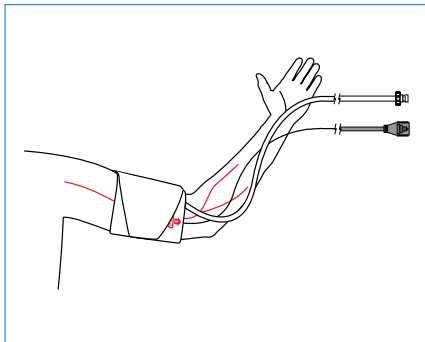


Step 6

Insert the microphone cable into the connector as shown below. The connectors can be inserted in any orientation. An audible click will be heard when a secure connection is made.

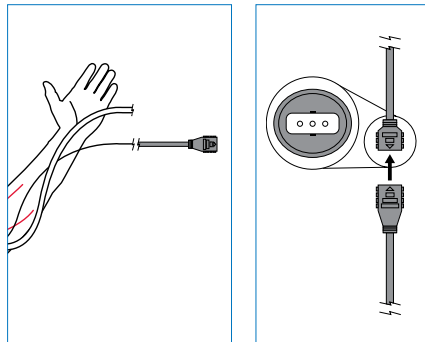

Step 7

Connect the cuff hose to the patient cable connector of the *Tango M2* patient cable as shown below.

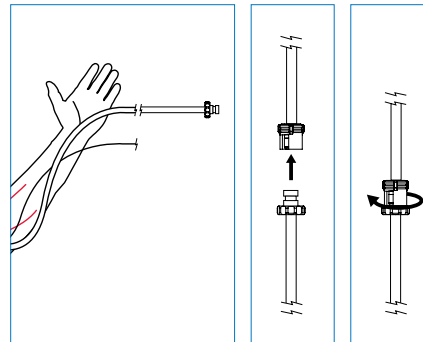

Step 8

Use the wrist straps provided with the *Tango M2* system to secure both the patient cable and the microphone cable to the patient's wrist as shown below.

